


PEPTIDE



COA TEST

Analytical Testing Laboratory
7271 Engle Rd Unit 201A, Middleburg Heights, OH 44130
sonic-laboratories.com

CERTIFICATE OF ANALYSIS

COA #: SD20260804_021_TZ30

SAMPLE INFORMATION

Client	Omega Labz	Accession #	SD20260804_021
Compound	Tirzepatide	Date Received	08/04/2026
Molecular Formula	C225H348N48O68	Date Reported	08/07/2026
Counter Ion / Salt	NA	Appearance	White lyophilized powder
Labeled Quantity	30 mg	Sample Form	Vial
Lot / Batch #	8500811510672	Storage	Room Temp
CAS Number	2023788-19-2	Crimp Color	Gray

All Chemical Analysis Performed by LC-MS/MS

ANALYTICAL RESULTS

Test / Analysis	Method	Specification	Result	Status
Identity (Mass Confirmation)	LC-MS/MS	Matches reference mass	Tirzepatide	Pass
Purity	LC-MS/MS	≥ 95.0%	99.69%	Pass
Net Peptide Content	LC-MS/MS	Report value	32.11 mg	Pass
Observed Molecular Mass	LC-MS	Within ± 1.0 Da	1204 [M+4H]	Pass
Theoretical Molecular Mass	Reference	—	4813.45 Da	Pass
Related Substances / Impurities	LC-MS/MS	Report value	Not Detected	Pass
Residual Solvents	LC-MS/MS	Report value	Not Detected	Pass

John Humes, MS.

John Humes, MS.

Analyzed by · Laboratory Analyst · 08/07/2026

Chetan Soni, PhD.

Chetan Soni, PhD.

Approved by · Laboratory Director · 08/07/2026


IMPORTANT NOTICE - FOR RESEARCH USE ONLY

This Certificate of Analysis is provided for informational and research purposes only. The sample(s) tested are intended solely for in vitro research, laboratory experimentation, and analytical reference use - not for human or animal consumption, medical diagnosis, therapeutic application, or any clinical use. Results apply only to the specific sample(s) submitted and tested. Unauthorized reproduction of this document is prohibited without written approval from Sonic Laboratories.


ANALYTICAL DATA

COA #: **SD20260804_021_TZ30**

CHROMATOGRAM

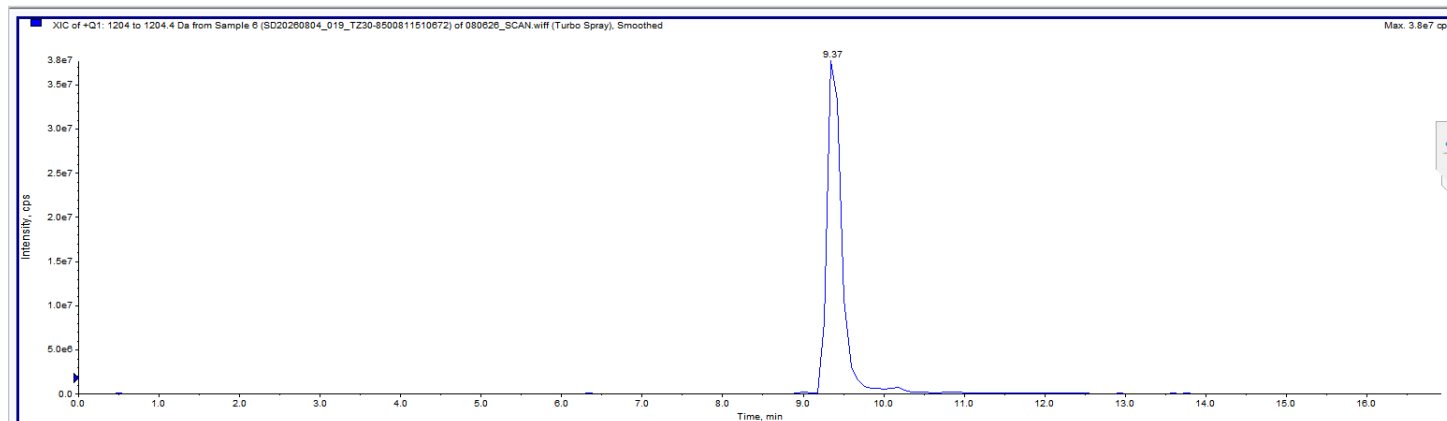

MASS SPECTRUM (LC-MS)

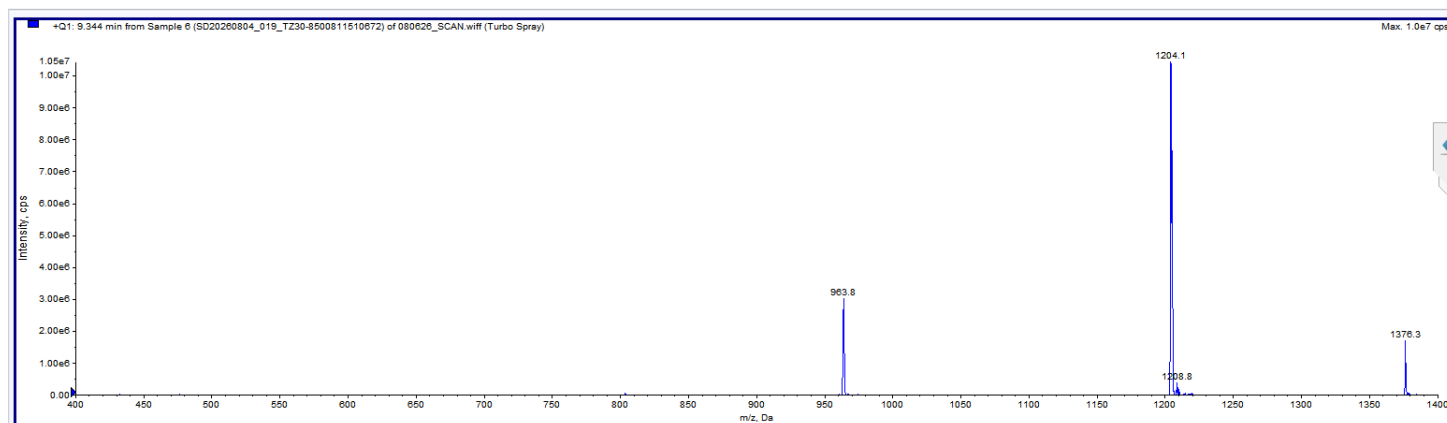

John Humes, MS. **John Humes, MS.**
Analyzed by · Laboratory Analyst · 08/07/2026

Chetan Soni, PhD. **Chetan Soni, PhD.**
Approved by · Laboratory Director · 08/07/2026

IMPORTANT NOTICE - FOR RESEARCH USE ONLY

This Certificate of Analysis is provided for informational and research purposes only. The sample(s) tested are intended solely for in vitro research, laboratory experimentation, and analytical reference use - not for human or animal consumption, medical diagnosis, therapeutic application, or any clinical use. Results apply only to the specific sample(s) submitted and tested. Unauthorized reproduction of this document is prohibited without written approval from Sonic Laboratories.

ANALYTICAL INTERPRETATION

Chromatogram

Retention Time Match

Mass Spectrum (LC-MS)

Identity (LC-MS, Q1 scan – Tirzepatide):

A positive-mode Q1 full scan acquired at 9.34min from the Tirzepatide sample shows a dominant precursor ion envelope centered around m/z 1204.1, with supporting peaks at 963.8, 1208.8, and 1376.3. These ions correspond to the expected multiply charged isotopic and adduct distribution of Tirzepatide under validated LC-MS conditions. The observed mass profile and charge-state pattern match the theoretical precursor ion distribution within tolerance limits, confirming analyte identity in this sample.

John Humes, MS.

John Humes, MS.

Analyzed by · Laboratory Analyst · 08/07/2026

Chetan Soni, PhD.

Chetan Soni, PhD.

Approved by · Laboratory Director · 08/07/2026

IMPORTANT NOTICE - FOR RESEARCH USE ONLY

This Certificate of Analysis is provided for informational and research purposes only. The sample(s) tested are intended solely for in vitro research, laboratory experimentation, and analytical reference use - not for human or animal consumption, medical diagnosis, therapeutic application, or any clinical use. Results apply only to the specific sample(s) submitted and tested. Unauthorized reproduction of this document is prohibited without written approval from Sonic Laboratories.